


# Selective 1D TOCSY

Selective 1D TOCSY  
using DPMOGE for selection  
Malose 3-ox 3-axis gradient probe

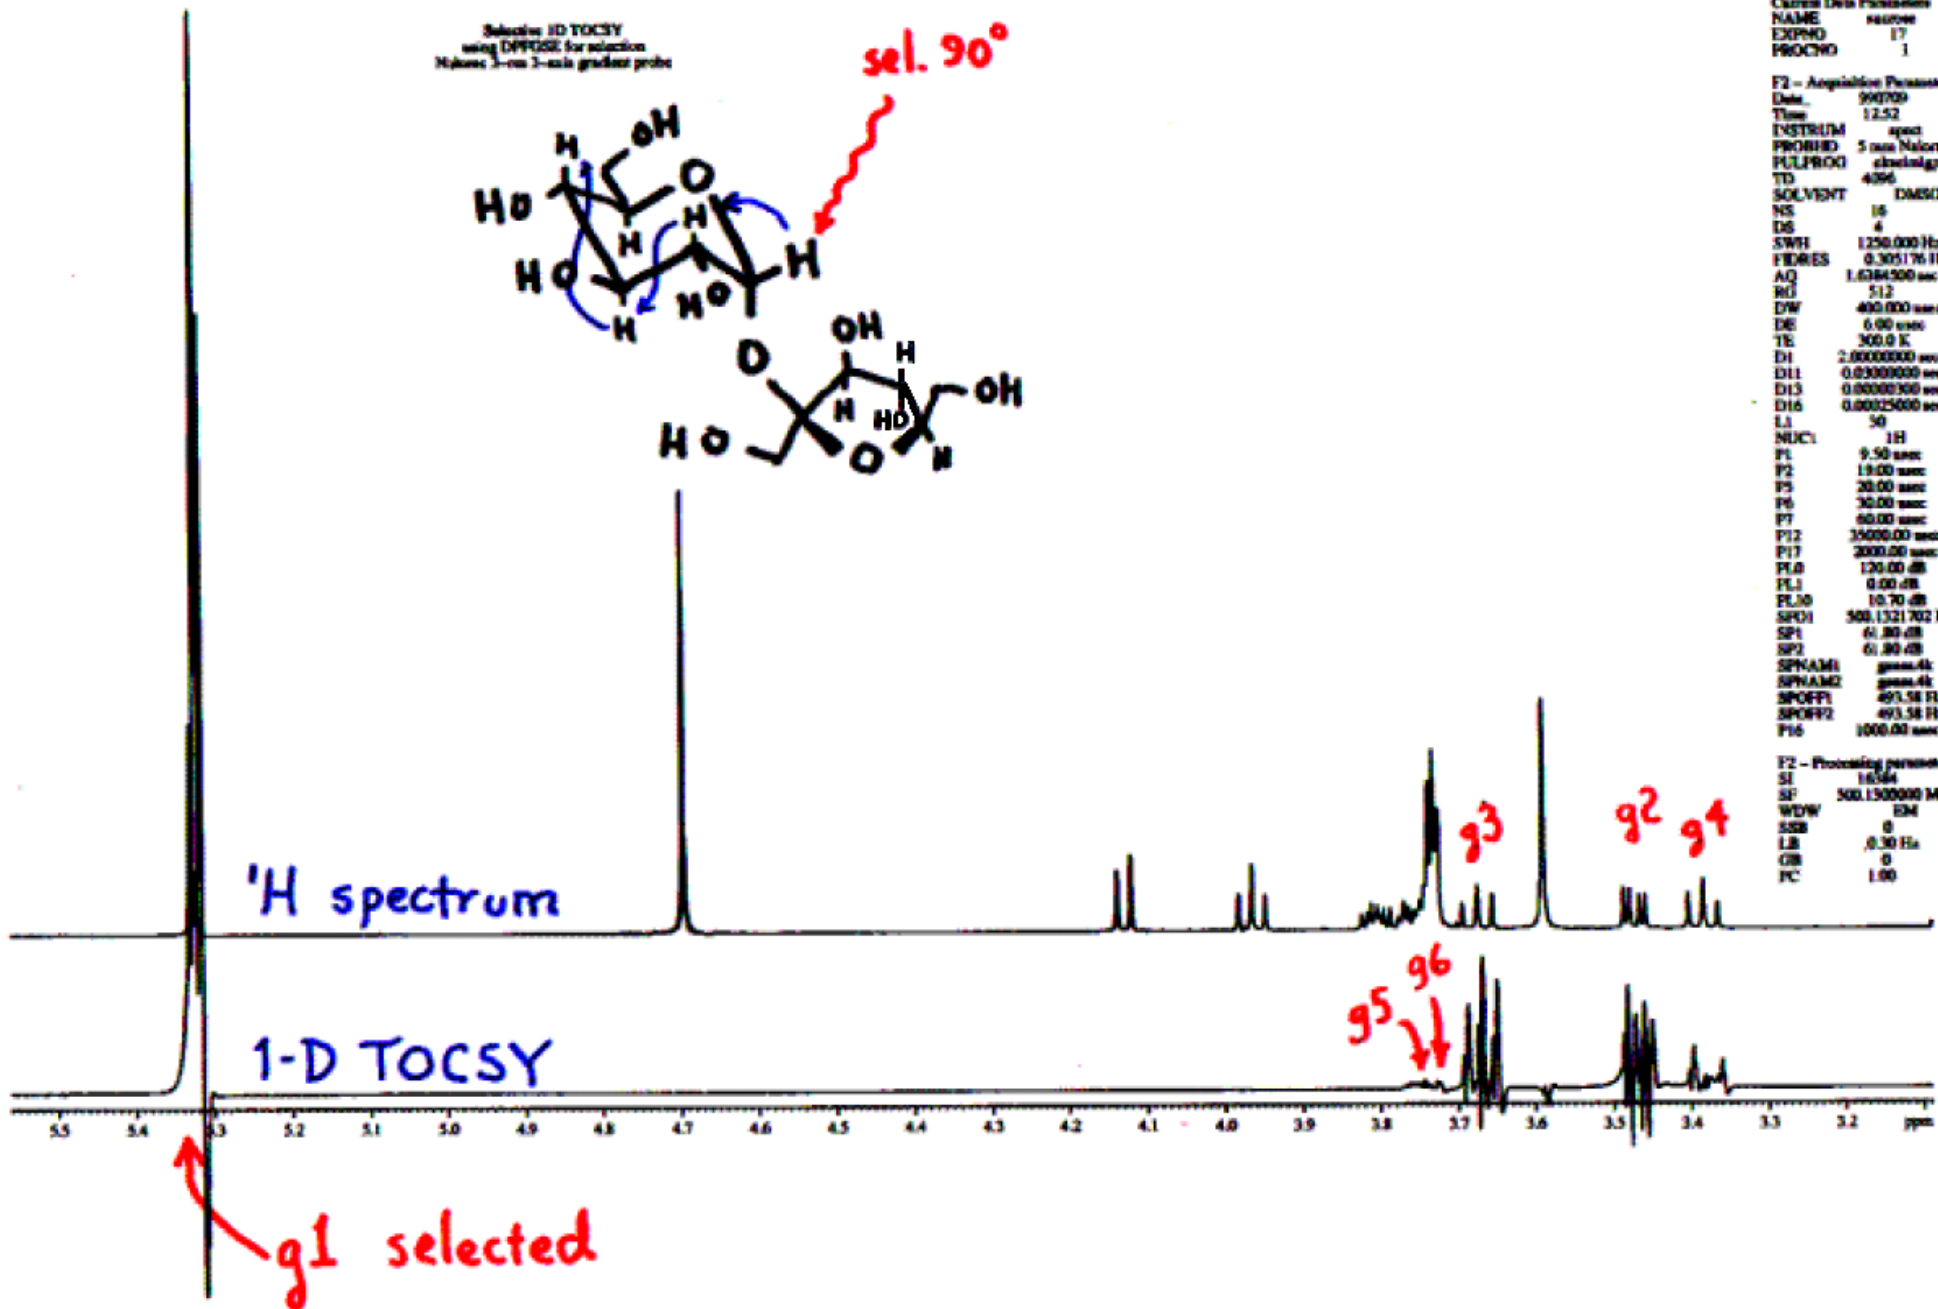

Current Data Parameters  
NAME sacrose  
EXPNO 17  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 900709  
Time 12.52  
INSTRUM spect  
PROBHD 5 mm Malonic  
PULPROG abnrd1gq  
TD 4096  
SOLVENT DMSO  
NS 16  
DS 4  
SWH 1250.000 Hz  
FIDRES 0.305176 Hz  
AQ 1.6384500 sec  
RG 512  
DM 400.000 usec  
DE 6.00 usec  
TE 300.0 K  
D1 2.0000000 sec  
D11 0.0000000 sec  
D13 0.0000000 sec  
D16 0.00025000 sec  
L1 50  
NUC1 1H  
P1 9.50 usec  
P2 19.00 usec  
P3 20.00 usec  
P6 30.00 usec  
P7 60.00 usec  
P12 35000.00 usec  
P17 2000.00 usec  
PL0 120.00 dB  
PL1 0.00 dB  
PL10 10.70 dB  
SFO1 500.1321702 MHz  
SF1 61.80 dB  
SF2 61.80 dB  
SFOA01 600.00  
SFOA02 600.00  
SFOFF1 493.58 Hz  
SFOFF2 493.58 Hz  
P16 1000.00 usec

F2 - Processing parameters  
SI 16384  
SF 500.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00